1/23




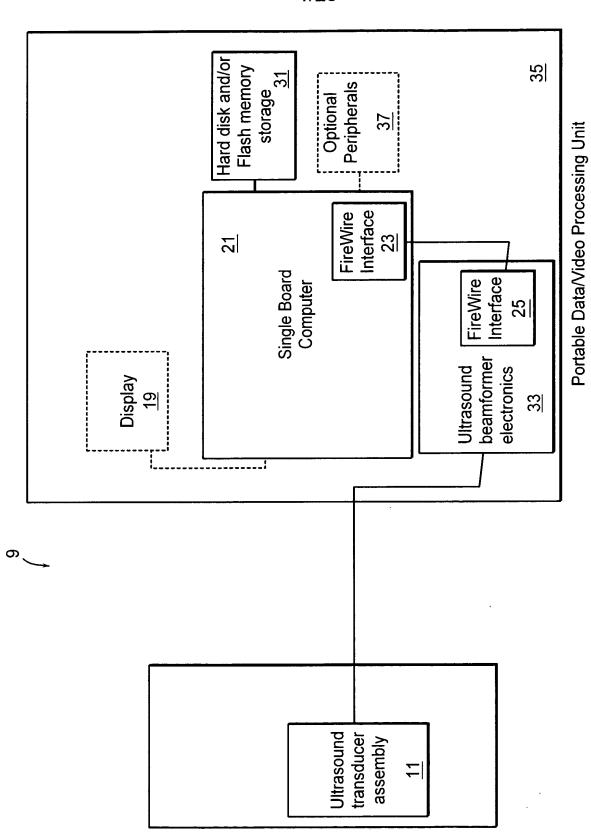



FIG. 1A

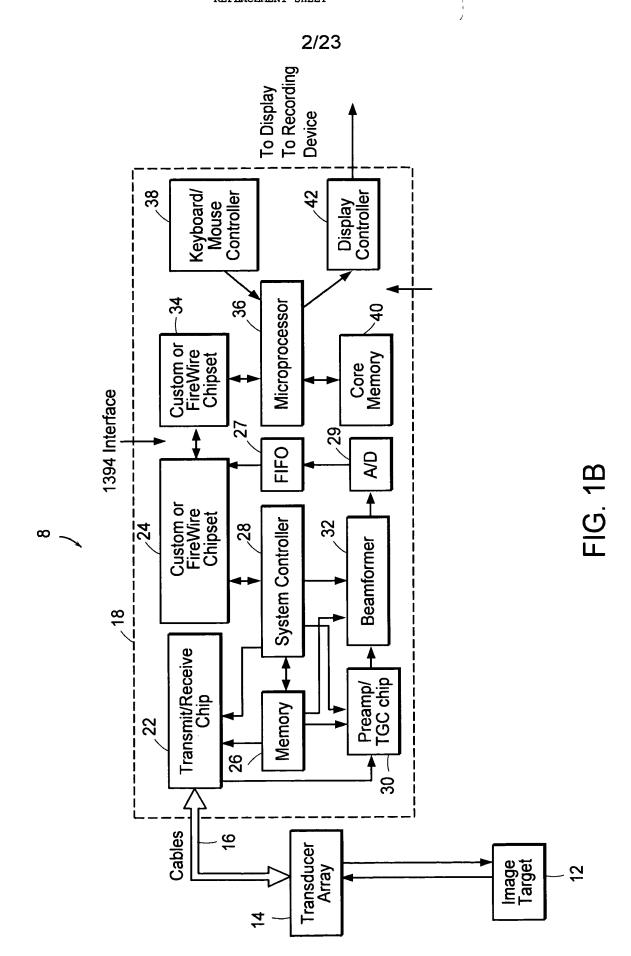

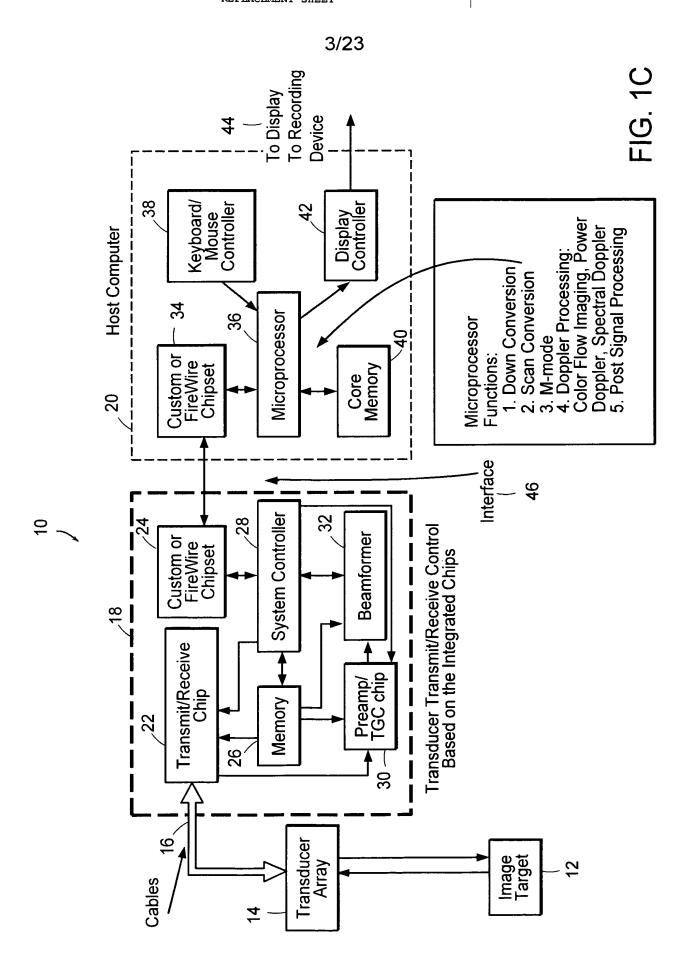

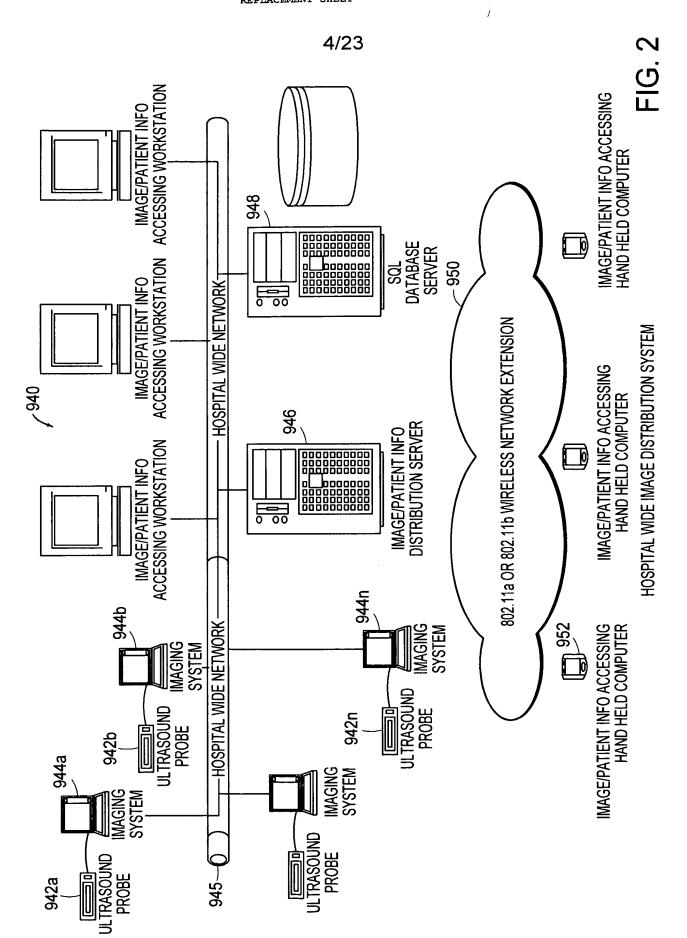

5/23

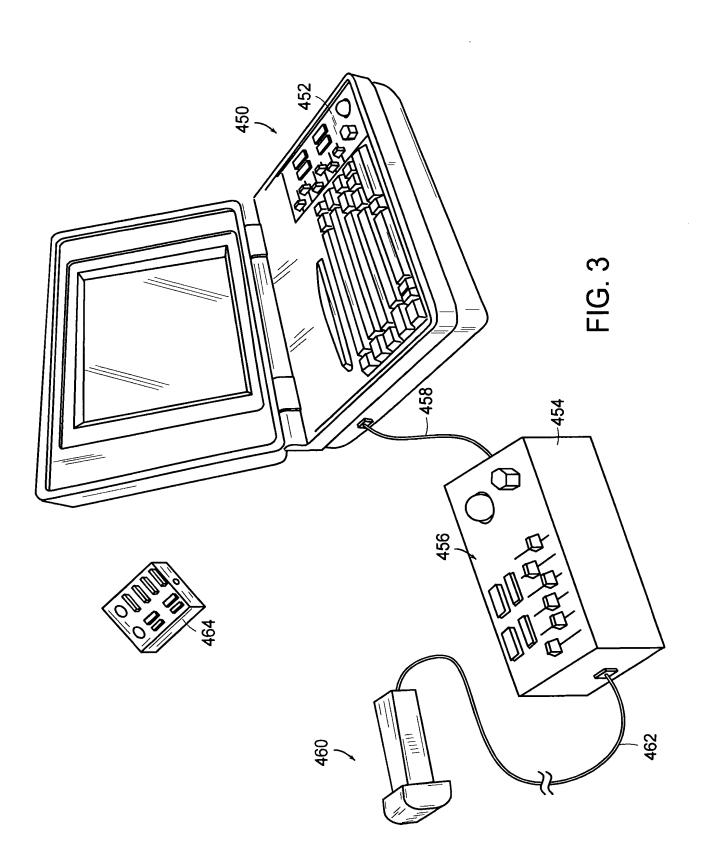

6/23 708 31.97 Hz 돌 S Patient Information File Edit View Exam/Measurements Controls Tools 902 Ultrasound 2-15-00 748 Tab 1 Tab 2 710 (F) Simulated Profile Data [Ultrasound] Depth 12 스 Focus 0.0 🗢 Œ 746 Ţgc For Help: press F1 Terason Bar <u>6</u> Start Start e

7/23

Apical Four-Chamber Duplex or Triplex Tissue Doppler Imaging

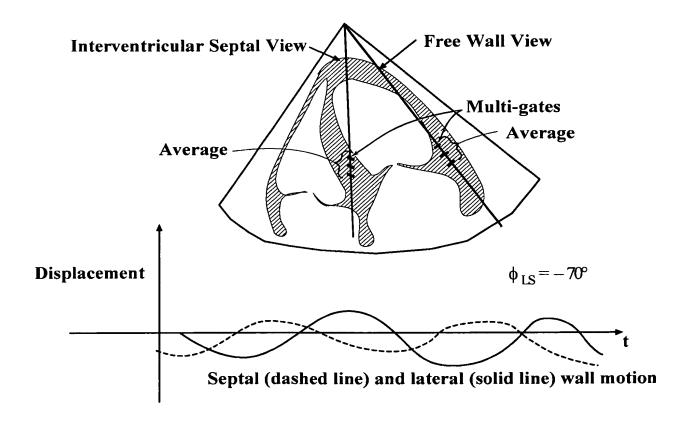


FIG. 5

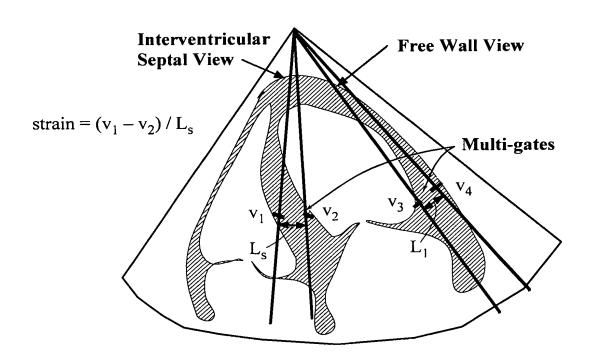


FIG. 6

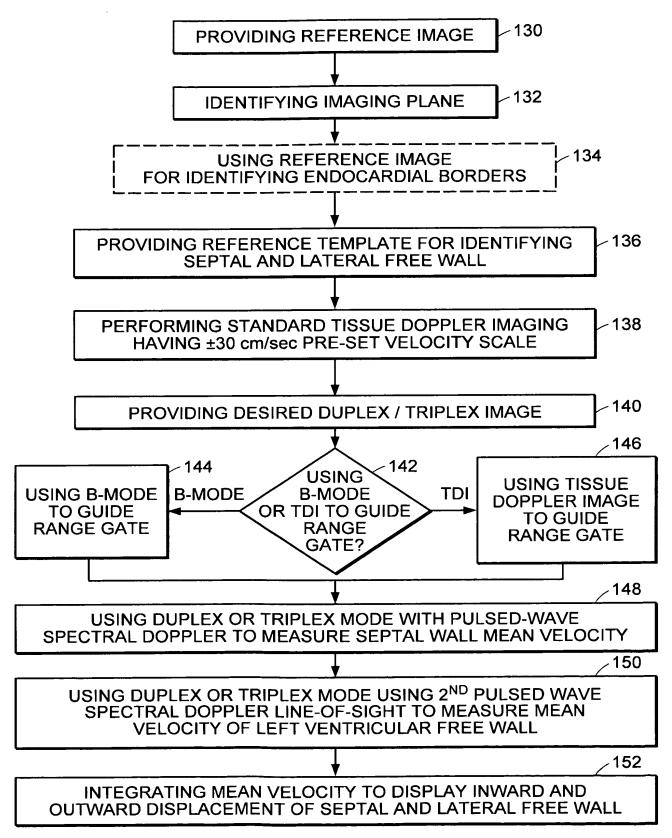


FIG. 7

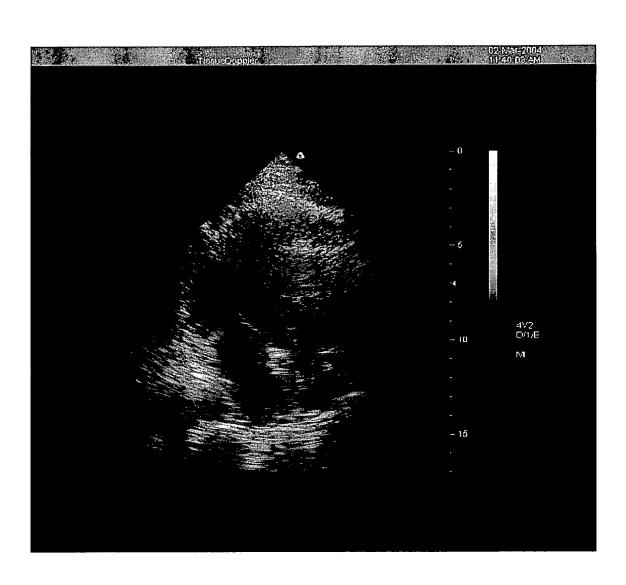


FIG. 8

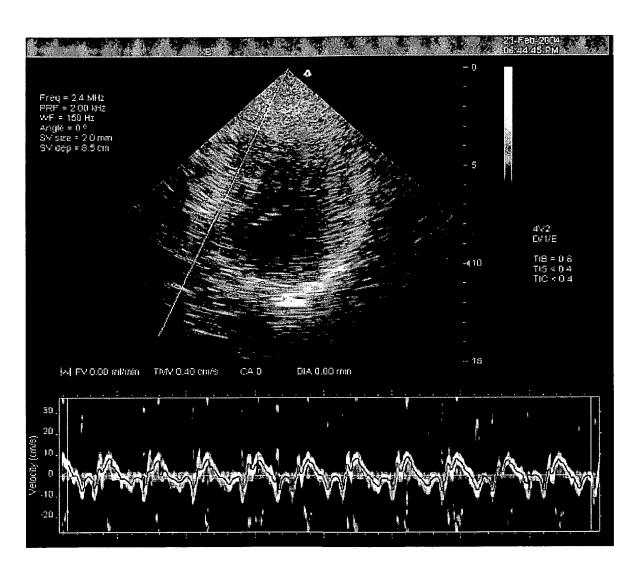


FIG. 9

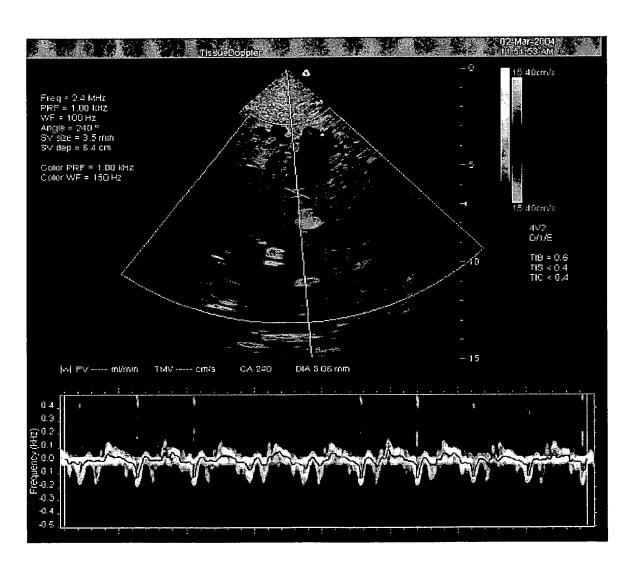


FIG. 10

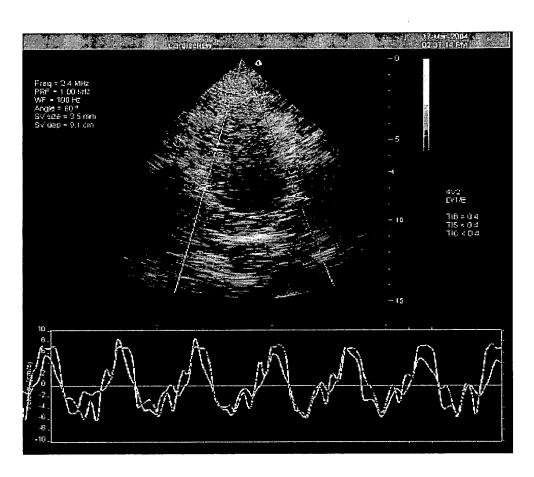


FIG. 11A

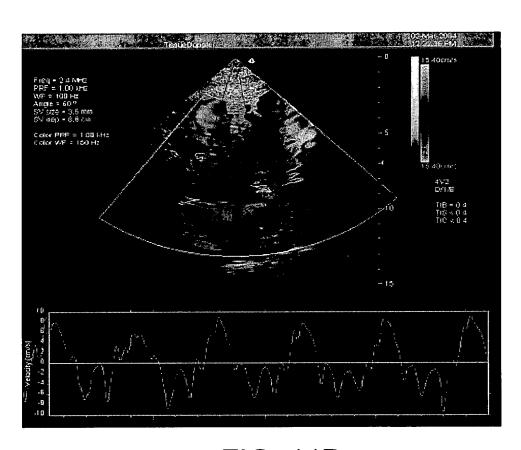


FIG. 11B

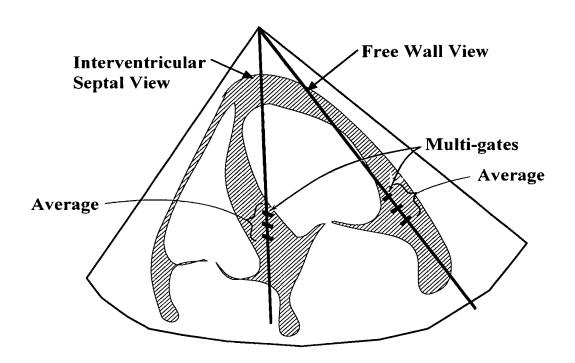


FIG. 12

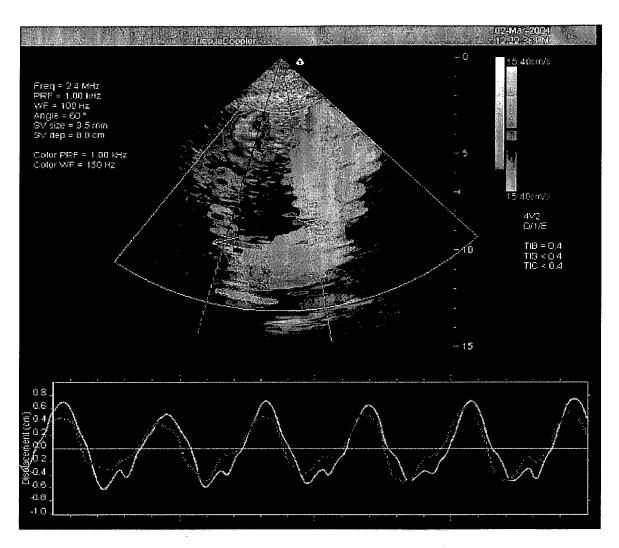


FIG. 13A

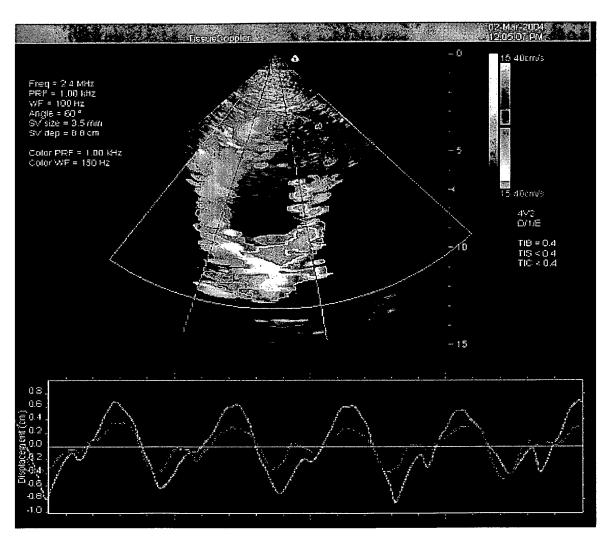


FIG. 13B

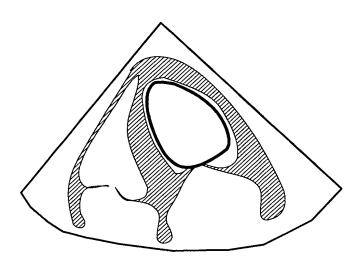


FIG. 14

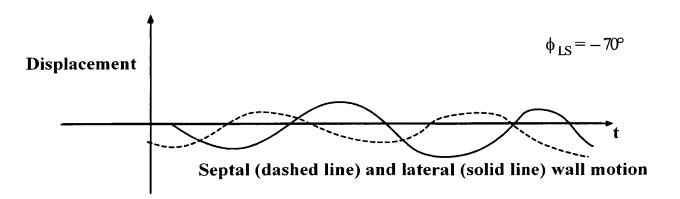


FIG. 15

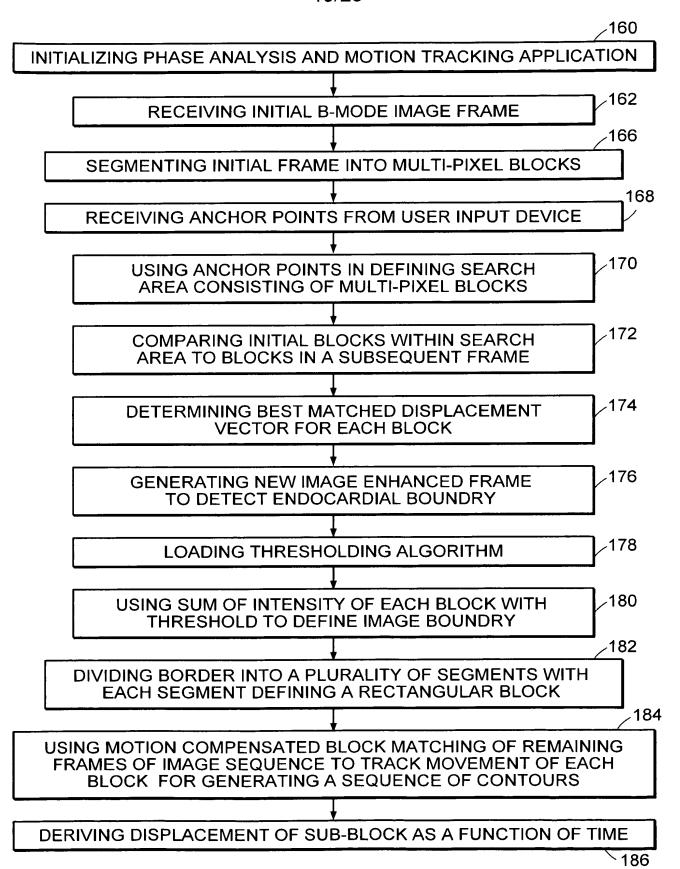


FIG. 16

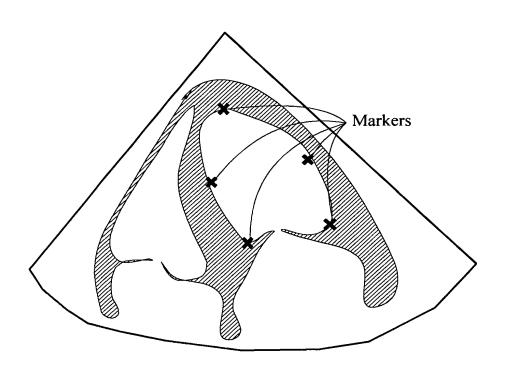


FIG. 17

21/23


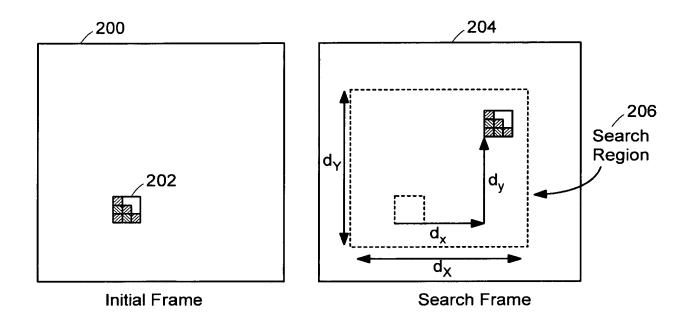



FIG. 18

FIG. 19

22/23

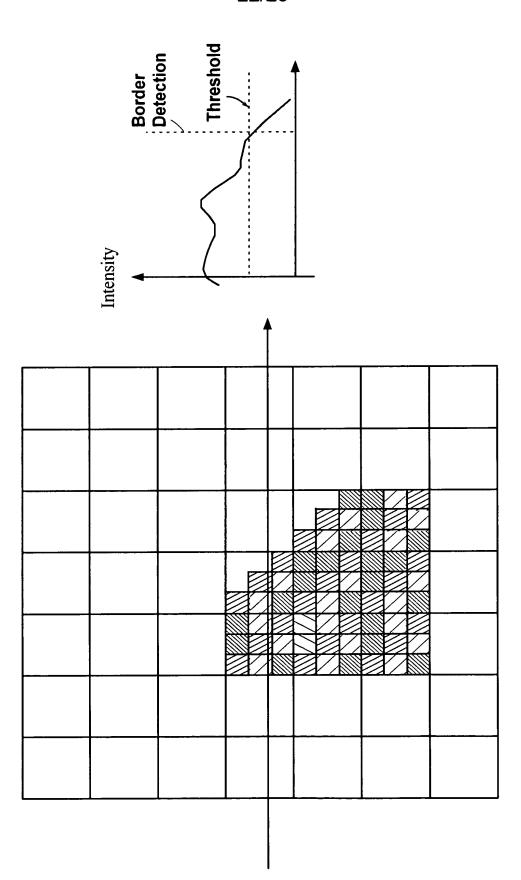

23/23

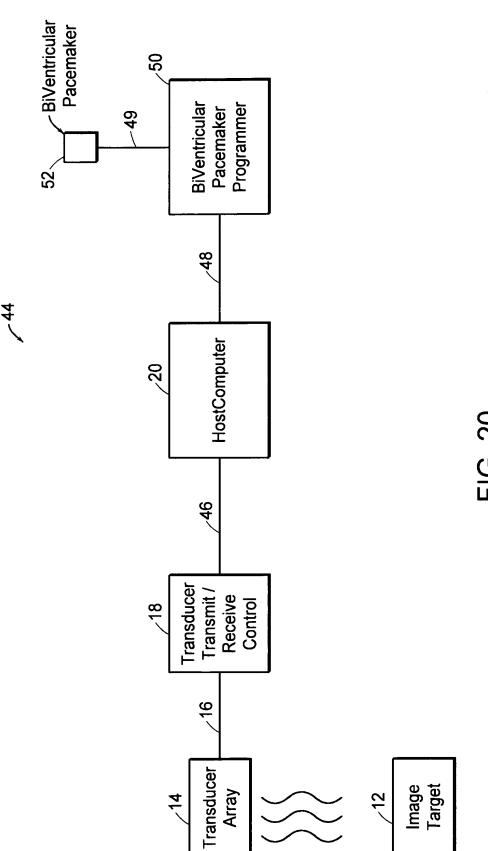

-16. 20